



Clinical
Services

Service User Guide

AMRA[®] BCP Scan

Powered by AMRA Profiler 4

Table of Contents

- About this Service User Guide5
 - Introduction5
 - Version History.....5
- About AMRA Profiler 47
 - Legal Manufacturer Information7
 - Intended Purpose (Canada).....8
 - Intended Use.....8
 - Medical Indications8
 - Metabolic diseases include8
 - Metabolic components of diseases8
 - Patient Population8
 - Contraindications8
- How to use AMRA® BCP Scan Service.....9
 - Requirements for Use9
 - Imaging Requirements9
 - Patient Data Requirements9
 - AMRA® MAsS Scan service has the following requirements on the input Patient Data:9
 - Data to Export9
 - Input of Patient Height on GE or Philips MRI Consoles.....10
 - Data Transfer10
 - Upload via Ambra Gateway10
 - Set-up.....11
 - Upload via Ambra Share Code11
 - Set-up.....11
 - Manual upload via Ambra Web Portal12
 - Set-up.....12
 - Browser Requirements.....12

Registration	12
Logging In.....	13
Uploading Studies	13
Download and View Reports	14
De-identification	15
Cybersecurity	15
Support.....	15
The AMRA® BCP Scan Report.....	16
Underlying Concepts	16
Reference Population	16
Virtual Control Group	16
Definitions of Measurements and Anatomical Regions.....	17
Anterior Thigh Muscle Group	17
Posterior Thigh Muscle Group	17
Muscle Fat	17
Muscle Volume	17
Visceral Fat	17
Subcutaneous Fat	17
Liver Fat	17
The Different Elements of the Report.....	18
1: Patient Data	19
2: Body Composition	19
Measurements.....	19
Bar plots	20
Handling of identified input data issues.....	20
Single leg used in case of identified issue in one of the legs	21
3: Coronal Images.....	21
4: Detailed Muscle Composition	21
Measurements.....	21
Bar plots	21
Handling of identified input data issues.....	21
5: Liver image	21
Issue Categories Explained	22

MRI Data Issues	22
Issue 1: Metal artifact	22
Issue 2: Motion during scan	22
Issue 3: Region partly outside field of view	22
Issue 4: Faulty alignment of adjacent slabs	23
Issue 5: Fat/water signal swap	23
Issue 6: Positive fat bias.....	23
Issue 10: Affected by strong negative fat signal.....	23
Issue 99: Other uncategorized issue.....	23
Patient Data Issues	24
Issue 11: Missing patient data.....	24
Issue 12: Unreasonable height or weight	24
Machine-readable Format	25
Reference Population Characteristics	26
Performance Specification	27
Appendix A: Input of Patient Height on GE or Philips MRI Consoles.....	28

About this Service User Guide

Introduction

This Service User Guide and the *DICOM Conformance Statement* are provided as electronic Instructions for Use at <https://amramedical.com/user-guides> upon your subscription purchase of AMRA® BCP Scan service.

This Service User Guide is a standalone document to be used for safe and effective operation of the AMRA® BCP Scan service powered by AMRA Profiler 4. This document describes how to use AMRA® BCP Scan, a service that is used to quantify global and regional fat volumes, fat fractions, and lean tissue volumes.

Version History

Version Number	Date of Revision	Updates since last version
1.0	2021-12-07	First version
2.0	2022-05-03	Updates: <ul style="list-style-type: none"> • <i>Data to Export</i> section <ul style="list-style-type: none"> ◦ Subsection <i>Input of patient height on the MRI console in case of GE or Philips</i> added • <i>Appendix A</i> added General: Minor clarifications in text and typo corrections.
3.0	2022-08-22	Updates: <ul style="list-style-type: none"> • <i>Body Composition</i> section, to cover improved issue notifications in the report: <ul style="list-style-type: none"> • A note is presented if Liver images were not received and Liver Fat measurement could not be calculated General: New AMRA logo and graphical profile. Minor clarifications. Images were updated to match the updated report.
4.0	2022-11-03	Updates: <ul style="list-style-type: none"> • <i>Patient Data Requirements</i> section added • <i>Manual upload via Ambra Web Portal</i> section <ul style="list-style-type: none"> ◦ Updated images from the Ambra web portal • <i>The Different Elements of the Report</i> section, image examples and text updated to match changes in report output: <ul style="list-style-type: none"> ◦ Minor layout change of bar plots ◦ Liver image is shown, without ROIs, in case Liver Fat value is not provided • <i>Issue Categories Explained</i> section <ul style="list-style-type: none"> ◦ Improved issue notifications and explanations
5.0	2022-12-20	Updates: <ul style="list-style-type: none"> • <i>Data Transfer</i> section updated to reflect that AMRA can now receive and send back protected health information • <i>Patient Data</i> section updated with Name

AMRA_BCP_Scan_Service_User_Guide_Canada_6.0 Created on 2023-04-12

6.0	2023-04-12	Updates: <ul style="list-style-type: none">• <i>Patient Data</i> section updated with DOB• <i>Machine-readable Format</i> section added
-----	------------	----------------------------------------------------------------------------------------------------------------------------------------------------------------

About AMRA Profiler 4

Legal Manufacturer Information

<p>Product Name: AMRA Profiler 4</p> <p>AMRA Profiler 4 is a medical device class I in Canada.</p>	<p>Manufacturer: AMRA Medical Badhusgatan 5 SE-582 22 Linköping SWEDEN www.amramedical.com support@amramedical.com</p>
<p>Clinical diagnosis should not be based solely on results shown in AMRA Profiler 4 reports.</p> <p>Results may vary slightly in different versions of AMRA Profiler 4.</p> <p>Any serious incident that has occurred in relation to the device should be reported to AMRA at support@amramedical.com and the competent authority of the Member State in which the healthcare institution and/or patient is established.</p>	

Intended Purpose (Canada)

Intended Use

AMRA Profiler 4 is a product for classification and quantification of global and regional fat volumes, fat fractions, and lean tissue volumes in comparison to normal ranges or control groups, using magnetic resonance (MR) data acquired with the Dixon water-fat imaging method. The measurement results are intended to assist in the diagnosis and monitoring of metabolic diseases, muscle diseases and metabolic components of diseases in a general population. Additionally, the measurements are intended to assist in the prediction, diagnosis, prognosis, and monitoring of adverse muscle composition, sarcopenia, and cachexia in populations with hepatic cirrhosis, chronic kidney disease, cancer, as well as before and after surgery such as organ transplant and gastric bypass. The medical device is solely to be used by trained professionals, qualified and certified by AMRA. The results are delivered in the form of a report including quantitative measurements and visualizations providing information for physicians' evaluation.

Medical Indications

- Health and wellness,
- Metabolic diseases,
- Muscle diseases,
- Metabolic components of diseases,
- Adverse muscle composition,
- Sarcopenia, and
- Cachexia.

Metabolic diseases include

- Cardiovascular disease,
- Coronary heart disease,
- Liver inflammation and fibrosis,
- Metabolic syndrome and related comorbidities,
- Non-alcoholic fatty liver disease (NAFLD), and
- Type 2 diabetes.

Metabolic components of diseases

Several diseases may have an effect on the fat and muscle compartments in the patient. This is detectable when the precision of the measurements are sufficiently high to assess, for example, longitudinal changes and treatment follow-up.

Patient Population

- General population, as well as in populations with
- Hepatic cirrhosis,
- Chronic kidney disease,
- Cancer, and
- Before and after surgery such as organ transplant and gastric bypass.

Contraindications

Not applicable, software only.

How to use AMRA[®] BCP Scan Service

Requirements for Use

AMRA[®] BCP Scan service has the following requirements for use:

- Ambra Health platform (DG PACS, 510(k) clearance: K152977), a web-based tool for data transfer, set-up to communicate with AMRA
- PDF-reader installed on the computer in order to read/view the AMRA[®] BCP Scan Report

Imaging Requirements

AMRA[®] BCP Scan service has the following requirements for the input DICOM data acquired with the magnetic resonance imaging (MRI) scanner:

- MRI scanner from one of the following manufacturers: GE, Siemens or Philips
- MRI images acquired with 1.5 T or 3.0 T main magnetic field strength
- 2-point Dixon data including fat, water, in-phase and opposed-phase images
- Images acquired with inherent transmit/receive body coil unless otherwise specified
- Neck-to-knee coverage in the head-feet direction, and field-of-view that covers subcutaneous tissue of the abdomen and thighs
- A voxel volume of minimum 1.75³ mm³
- A voxel volume of maximum 4.5³ mm³
- An overlap between neighbouring slabs of at least 3 cm
- T1-weighted images with a flip angle of 10 degrees and short repetition time
- DICOM files as an archive compliant with the *DICOM conformance statement*
- Fat, water, in-phase and opposed-phase image separation identifiable by Series Description or Image Type DICOM tags
- For liver fat assessment: Scanner manufacturer's clinical liver application images acquired with factory settings including fat fraction, fat, water and T2*/R2* images, or a multi-echo gradient-echo acquisition of the liver with at least 3 in-phase echo times

Patient Data Requirements

AMRA[®] MAsS Scan service has the following requirements on the input Patient Data:

- Patient Height shall be measured to the closest cm or half-inch
- Patient Weight shall be measured to the closest kg or lbs
- Patient Sex shall be provided
- Patient Age shall be provided

For detailed information on the required DICOM information, please refer to the *DICOM Conformance Statement* provided at <https://amramedical.com/user-guides>.

Data to Export

The below list describes which data needs to be exported for transfer to Ambra Health.

- Body-slabs: Export fat, water, in-phase and opposite-phase images
- Liver image acquisition for liver fat: Export fat, water, fat fraction and R2* images, as well as in-phase/opposite-phase (GE/Philips) or Original echoes (Siemens)
- Note that compression or enhanced DICOM are not supported

- Transfer complete datasets, including body slabs and liver slabs as one study
- If alternative liver image acquisition for liver fat, T2s (T2*), is used, export all corresponding images (multi-echo series or separate spoiled GRE images with different TEs)

Exported DICOM files must comply with the *DICOM Conformance Statement* that can be found at <https://amramedical.com/user-guides>. Note, that information on the patient’s sex, height and weight needs to be included in the exported DICOM data. This information is typically typed in at patient registration on the MRI console.

Input of Patient Height on GE or Philips MRI Consoles


In case of GE or Philips scanners, there is no dedicated field to input patient height on the MRI console. The recommended solution is then to add the height information in the tags Study Comments (Philips) or Additional Patient History (GE) instead. A guide on how to enter the height information in order for the information to be correctly interpreted and used by AMRA can be found as a printable sheet in Appendix A. If manual data upload through Ambra Web Portal is used, the patient height can be input in the Ambra Web Portal instead.

Data Transfer

AMRA uses the Ambra Health platform for data transfer. AMRA recommends that one of the following three transfer solutions are used to upload the data to the Ambra Cloud; direct upload from PACS via Ambra Gateway, transfer between Ambra accounts via share code, or manual upload to the Ambra Web Portal. In this chapter, “report” refers to the BCP Scan Report.

Upload via Ambra Gateway

This is the flow-chart of the setup when using upload from PACS via Ambra Gateway.

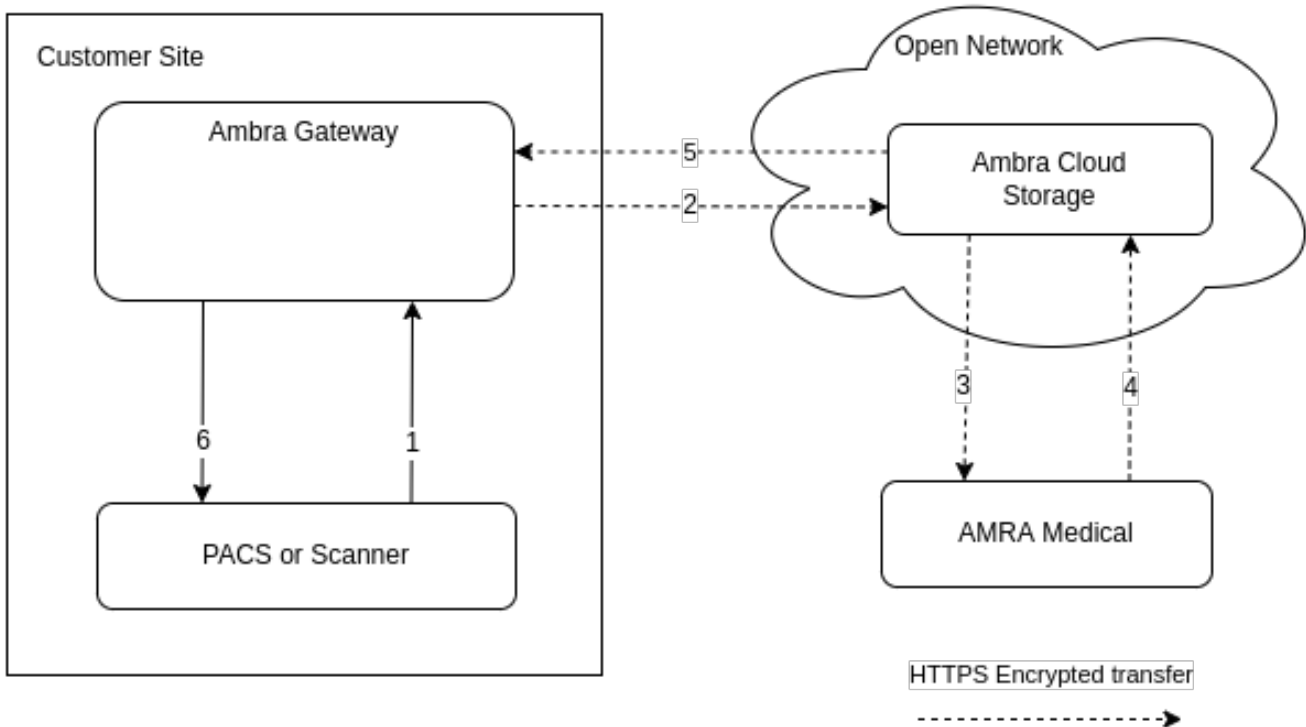

Automatic data transfer via Ambra Gateway contains the following steps:

1. Push of DICOM images, including sex, weight and height of the patient, from PACS or MRI scanner to the Ambra Gateway
2. Automatic upload of images to Ambra Cloud Storage

3. Automatic download of images to AMRA
4. A PDF report is returned to Ambra Cloud Storage
5. Automatic download of report to Ambra Gateway
6. Automatic push of the report to the patient exam in PACS

Set-up

For setup of the Ambra Gateway solution, contact your PACS or IT administrator.


The following procedures are needed for the setup of Ambra Gateway.

- A physical PC or virtual machine, on which the gateway can be installed, set up as a DICOM node on the same network as the PACS and/or MRI scanner.
- Configuration of a new DICOM route in the PACS or MRI scanner, so that images can be pushed to the gateway.
- The IP address, port and AE Title to be used by the gateway.
- The current IP address, port and AE Title used by the PACS.

Note that there is a possibility to get a notification if data was not possible to upload from Ambra Gateway to the Ambra cloud. It is recommended that this notification is enabled at all times and that the receiver(s) of this notification is specified and communicated to Ambra Health at set-up.

Upload via Ambra Share Code

This transfer option can be selected if the site is already using Ambra and have an account. The data transfer can then be done via share code in the Ambra cloud. This is the flow-chart when using upload via Ambra Share Code.

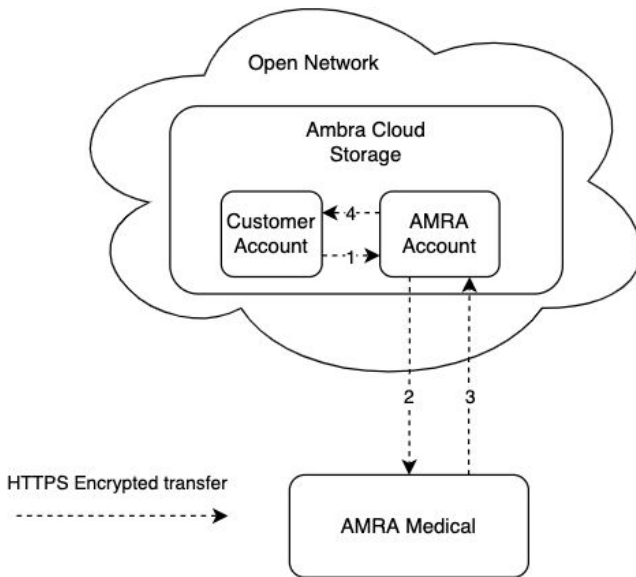

Automatic data transfer via Ambra Share Code contains the following steps:


1. DICOM images, including sex, weight and height of the patient, are shared to AMRA's Account, via share code and the routing rule set up
2. Automatic download of DICOM images to AMRA
3. Automatic upload of the report to AMRA's Account
4. Automatic share of the report to the Customer's Account, via share code and routing rule set up

Set-up

For set-up of the Ambra Share Code solution, a share code and routing rule needs to be setup for the Customer Account as well as for the AMRA account in Ambra cloud. Contact your local PACS or IT administrator.

Manual upload via Ambra Web Portal

This is the flow-chart for manual upload to Ambra Web Portal.

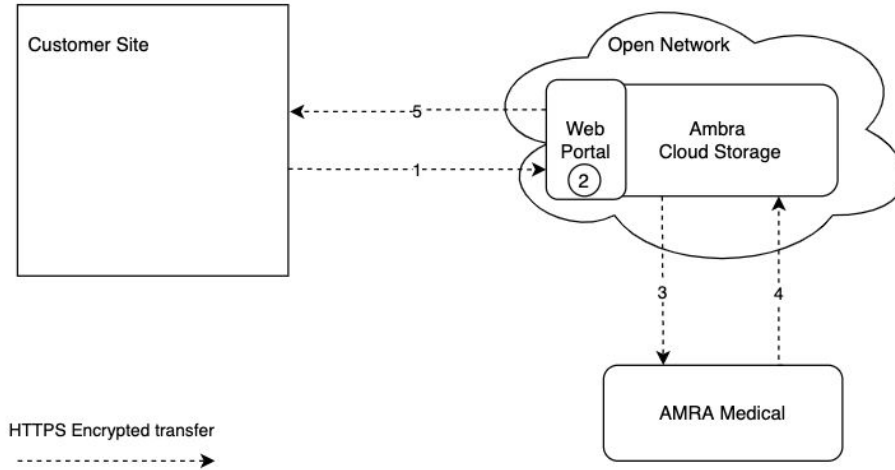

Manual data transfer via Ambra Web Portal contains the following steps:

1. DICOM images, including sex, weight and height of the patient, are manually uploaded to the Ambra Web Portal
2. Patient ID, sex, height and weight can be modified in the web portal, if needed
3. Automatic download of DICOM images to AMRA
4. Automatic upload of the report to Ambra Cloud Storage
5. Manual download of the report from the Ambra Web Portal

Set-up

The only requirement to upload images manually to Ambra is a computer with Internet access. Browser requirements and instructions for the different steps (registration, log in, upload, download and view reports) are described later in this chapter.

Browser Requirements

Recommended browser: Google Chrome

Other compatible browsers: Microsoft Internet Explorer 9 or later, Microsoft Edge, Apple Safari and Firefox.

Registration

You will be sent an e-mail invite where you will be asked to register for the Ambra platform. The invite is sent from support@amramedical.com, please check your spam folder if you haven't received the invite after service subscription startup.

Logging In

To log in, go to: <https://amra.ambrahealth.com/>
Your email address will be your Login.

Sign In

Login


Password

[Forgot your password?](#)

Sign In


Uploading Studies

1. From the Studies drop-down, select the appropriate location/site.

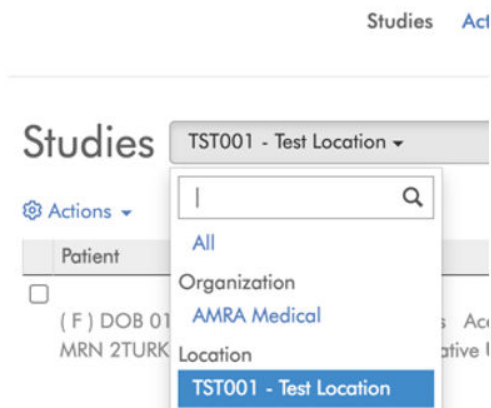

You will only see the locations that are relevant to your studies. In the startup email, you will receive information about the location name.

2. Click 'Add Study' then 'Upload Studies'.

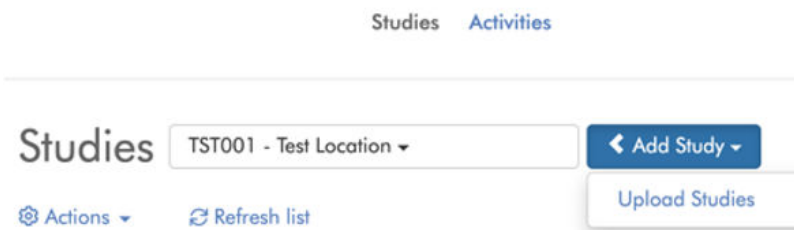

- During manual upload you will have the chance to update specific DICOM tags. The resulting report will be based on the given metadata in these fields, so make sure that they are correct.

Choose studies to upload

[Choose File...](#)

Description	Images	Patient Name	DOB	Modality	Study Date	
<input checked="" type="checkbox"/> Certification scan	96	Anon	1990-01-01	MR	2015-09-29	

Patient ID

New Patient ID

Patient Size

New Patient Size

Enter the patient's size (##.##) in meters.

Patient Sex

New Patient Sex

Patient Weight

New Patient Weight

Enter the patient's weight (###.#) in kilograms.

Please note, that any changes done after upload will not automatically be transferred to us. Please email support@amramedical.com alerting us to any changes.

For more help uploading, please consult Ambra's Help Center: support.ambrahealth.com

Download and View Reports

When patient data has been analyzed and results are available, you will receive an e-mail notification. You can then log-in and view/download the report. This is best accomplished with Chrome.

- From Studies drop-down, select the appropriate site/location.
- To view, click on the Reports icon from the Actions on the right-hand side of the study in the worklist.

Uploaded	Actions
08-16-2022 08:07 AM	Images Edit Download Reports Latest Report
<div style="border: 1px solid #ccc; padding: 5px; margin-top: 10px;"> <p>blank.pdf</p> <p>From: TST001 - Test Location</p> <p>Uploaded: 08-17-2022 04:37 AM</p> </div>	

- Double click the desired report to download.

De-identification

Sometimes, it is wanted to have the data de-identified before upload, so that no protected health information is sent. In this case, the site is responsible for the de-identification of the data.

When using the Ambra Gateway solution, the de-identification can be done either before the data is pushed to the gateway, or within the gateway. If it is done within the gateway, the site needs to agree with Ambra at set up, on which DICOM tags shall be de-identified.

When using the Ambra Share code solution, the de-identification of data shall be done before data is pushed to the AMRA Account. The site needs to agree with Ambra at set up, on which DICOM tags shall be de-identified.

When using the Manual Upload solution, the de-identification of data shall be done before data is uploaded to the Ambra Web Portal. Additionally, AMRA's back-up de-identification can be activated at startup of service.

The *DICOM Conformance Statement* states which DICOM tags are required in order to generate the BCP Scan Report output. AMRA will not actively screen for protected health information in the received data.

Cybersecurity

The BCP Scan report requires an installed PDF-reader on a computer in order to read/view the Report. This computer should have an operating system and a viewer kept up to date as well as an updated anti-virus software. Please contact your local system administrator should you have any questions regarding cybersecurity measures or if you suspect any cybersecurity incidents.

Support

If you have any questions, please contact AMRA at support@amramedical.com.

The AMRA[®] BCP Scan Report

This chapter provides the user of the AMRA[®] BCP Scan report with more detailed information on the underlying concepts, measurement definitions, how to interpret the different elements of the report, and how issues in input data are handled.

Underlying Concepts

Reference Population

In the AMRA[®] BCP Scan, a reference population of more than 30,000 individuals is used. Each individual in this reference population has its own set of Patient Data (height, weight, sex) and body composition measurements calculated by AMRA. The reference population is used to put the patient in a relevant context that is helpful when assessing his/her data.

Virtual Control Group

The patient specific virtual control group is extracted from the reference population by finding a group of individuals with the same sex and similar body size ($BMI \pm 2 \text{ kg/m}^2$) as the patient. With this, each patient that gets a BCP Scan will get their own individualized reference group. The virtual control group is created based on the Patient Data (height, weight and sex information) that is provided in conjunction with the upload of MRI data to Ambra Health.

The patient specific virtual control group is used in the report to present an individualized statistical reference (blue field) in the bar plots in the report. The blue field represents the interquartile range (25th-75th percentile) of the virtual control group and is given as a reference to help assess if the patient's value is within the statistically expected range, given its sex and body size.

Note: The patient marker being within the blue field, does not indicate if the patient is healthy or unhealthy.

Note: If a patient has been scanned at two different timepoints, and a comparison of reports between these timepoints are made, the virtual control group and thus the blue field in bar plots can differ between the reports. For instance, if the patient has increased his/her weight between the two scans, the individuals included in the patient specific virtual control group will be slightly different between the timepoints and thus the resulting blue field will have a different distribution.

Definitions of Measurements and Anatomical Regions

Anterior Thigh Muscle Group

Includes quadriceps femoris, sartorius and tensor fascia latae.

Posterior Thigh Muscle Group

Includes gluteus muscles, iliacus, adductor muscles and hamstring muscles.

Muscle Fat

Muscle Fat is the fraction of adipose tissue in the muscle, also known as muscle fat infiltration or intramuscular fat. Defined as the average proton density fat fraction within the Muscle Volume. Muscle Fat is measured in percentages (%).

Muscle Volume

The fat-free muscle volume, i.e. the volume of active tissue in the muscle. Defined as the volume of all voxels with fat fraction <50%. Muscle Volume is measured in liters (L).

Visceral Fat

Defined as the volume of adipose tissue within the abdominal cavity, excluding adipose tissue outside the abdominal skeletal muscles and adipose tissue and lipids within the cavity and posterior of the spine and back muscles. Visceral Fat is measured in liters (L).

Subcutaneous Fat


Defined as the subcutaneous adipose tissue volume in the abdomen from the top of the femoral heads to the top of the thoracic vertebrae, T9. Subcutaneous Fat is measured in liters (L).

Liver Fat

Defined as the average proton density fat fraction in regions of interest in the liver. Liver Fat is measured in percentages (%).

The Different Elements of the Report

The BCP Scan report contains several different elements, which are described in this section.

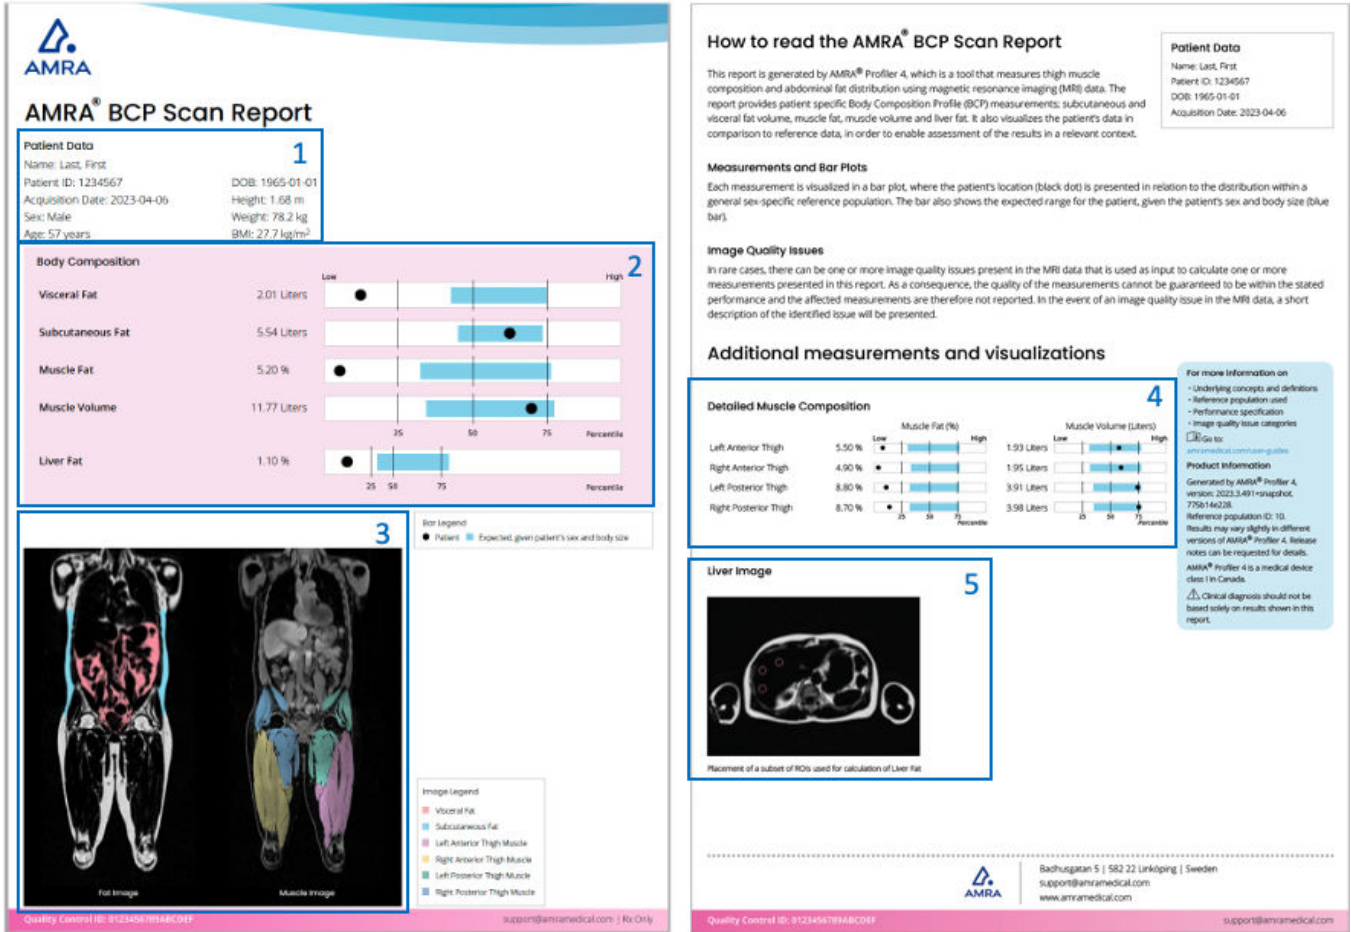

AMRA® BCP Scan Report

1 Patient Data
 Name: Last, First
 Patient ID: 1234567
 Acquisition Date: 2023-04-06
 Sex: Male
 Age: 57 years
 DOB: 1965-01-01
 Height: 1.68 m
 Weight: 78.2 kg
 BMI: 27.7 kg/m²

2 Body Composition

Measurement	Value	Visual Representation
Visceral Fat	2.01 Liters	Bar chart showing patient value (black dot) at approximately 25% percentile.
Subcutaneous Fat	5.54 Liters	Bar chart showing patient value (black dot) at approximately 65% percentile.
Muscle Fat	5.20 %	Bar chart showing patient value (black dot) at approximately 25% percentile.
Muscle Volume	11.77 Liters	Bar chart showing patient value (black dot) at approximately 75% percentile.
Liver Fat	1.10 %	Bar chart showing patient value (black dot) at approximately 25% percentile.

3 Fat Image / Muscle Image

Image Legend:
 ● Patient ● Expected, given patient's sex and body size

Image Legend:
 ● Visceral Fat
 ● Subcutaneous Fat
 ● Left Anterior Thigh Muscle
 ● Right Anterior Thigh Muscle
 ● Left Posterior Thigh Muscle
 ● Right Posterior Thigh Muscle

4 Detailed Muscle Composition

Muscle Group	Muscle Fat (%)	Muscle Volume (Liters)
Left Anterior Thigh	5.50 %	1.93 Liters
Right Anterior Thigh	4.90 %	1.95 Liters
Left Posterior Thigh	8.80 %	3.91 Liters
Right Posterior Thigh	8.70 %	3.98 Liters

5 Liver Image

Placement of a subset of ROIs used for calculation of Liver Fat.

How to read the AMRA® BCP Scan Report

This report is generated by AMRA® Profiler 4, which is a tool that measures thigh muscle composition and abdominal fat distribution using magnetic resonance imaging (MRI) data. The report provides patient specific Body Composition Profile (BCP) measurements; subcutaneous and visceral fat volume, muscle fat, muscle volume and liver fat. It also visualizes the patient's data in comparison to reference data, in order to enable assessment of the results in a relevant context.

Patient Data
 Name: Last, First
 Patient ID: 1234567
 DOB: 1965-01-01
 Acquisition Date: 2023-04-06

Measurements and Bar Plots
 Each measurement is visualized in a bar plot, where the patient's location (black dot) is presented in relation to the distribution within a general sex-specific reference population. The bar also shows the expected range for the patient, given the patient's sex and body size (Blue bar).

Image Quality Issues
 In rare cases, there can be one or more image quality issues present in the MRI data that is used as input to calculate one or more measurements presented in this report. As a consequence, the quality of the measurements cannot be guaranteed to be within the stated performance and the affected measurements are therefore not reported. In the event of an image quality issue in the MRI data, a short description of the identified issue will be presented.

Additional measurements and visualizations

For more information on
 - Underlying concepts and definitions
 - Reference population used
 - Performance specification
 - Image quality issue categories

Go to: [amramedical.com/ugp-guides](#)

Product Information
 Generated by AMRA® Profiler 4, version: 2023.3.491 +supplbot, 7759146238.
 Reference population ID: 10.
 Results may vary slightly in different versions of AMRA® Profiler 4. Release notes can be requested for details.
 AMRA® Profiler 4 is a medical device class 1 in Canada.
 ⚠️ Clinical diagnosis should not be based solely on results shown in this report.

Quality Control ID: 8123456789ABCDEF | support@amramedical.com | For Only

The BCP Scan report, with references to the following descriptions of each element (1-5).

1: Patient Data

The Patient Data element presents the patient specific metadata. This data is used as ground for the visual elements presented in the report.

Information	Source of information (DICOM tag or other)	Possible to modify in case of manual upload (YES/NO)
Name	(0010, 0010) Patient's Name	YES
DOB	(0010,0030) Patient's Birth Date	YES
Patient ID	(0010,0020) Patient ID	YES
Acquisition Date	(0008,0022) Acquisition Date Attribute	NO
Sex	(0010,0040) Patient's Sex	YES
Age	(0010,1020) Patient's Age	NO
Height	(0010,1020) Patient's Size (m)	YES
Weight	(0010,1030) Patient's Weight (kg)	YES
BMI	Weight / Height ² (kg/m ²) Calculated by AMRA, given the received Weight and Height numbers.	NO

In case any of the Patient Data was omitted at upload, the value is replaced by a dash “–” in the Patient Data element. Specifically, in case height, weight or sex is omitted, the bar plots are presented blank in the BCP Scan report.

Note that the Name and DOB (Date of Birth) fields can be configured to not be output. This is configured at startup of service.

The Patient ID tag needs to be populated with a string or number, unique for the patient, that is easily accessible for the site. It will be used to identify a specific dataset when AMRA communicates with you. Always refer to the Patient ID if there is a need to contact AMRA support about a specific examination.

2: Body Composition

Measurements

The body composition measurements give an objective measure of the fat distribution and muscle composition within the patient's body, allowing for assessment of body composition changes and early signs of treatment impact. The measurements may assist in diagnosis, prediction and monitoring of metabolic diseases.


Higher fraction of abdominal fat consisting of Visceral Fat indicates an unfavorable fat distribution associated with increased cardiac risk. Patients presenting with high Visceral Fat and low Liver Fat, have a higher risk for a cardiac event. Visceral Fat has further been associated with certain types of cancer, liver inflammation and fibrosis.

The Muscle Fat measurement is calculated as the mean muscle fat infiltration in the anterior thigh muscle groups in both legs. A high value means there is a higher fraction of fat in the muscles, which indicates a lower muscle quality and function. The

Muscle Volume measurement is calculated as the thigh fat-free muscle volume of both the anterior and posterior thigh muscle groups. A low value may indicate that there is low quantity of fat-free muscle tissue.

Bar plots

Each body composition measurement is visualized in a bar plot to help put the patient’s measurement in a relevant context. The patient’s measurement (black dot) is compared to the distribution of measurements within a sex specific reference population (white bar). The 25th, 50th and 75th percentiles of this reference population are presented as solid lines. The distribution within the patient’s virtual control group (blue bar) shows the expected range of the measurement, given the provided patient’s sex and body size at time of scan.



Example: The patient’s Muscle Volume is slightly below the median among individuals in the reference population with the same sex (below the 50th percentile). The Muscle Volume is within what could be expected, given the patient’s sex and body size (within the blue field), however, often individuals similar to him/her has a higher Muscle Volume (patient is in the left end of the blue field).


Liver fat has a skewed distribution in a general population, where most individuals have little liver fat. Therefore, the Liver Fat bar plot is scaled differently than the other bars plots, for easier interpretation.

Note: The patient marker being within the blue field, does not indicate if the patient is healthy or unhealthy.

Handling of identified input data issues

If issues in the MRI data are identified, the quality of the measurements cannot be guaranteed to be within the stated performance and the affected measurement(s) are therefore not reported. This is indicated by a dash, “–”, instead of a value and a blank bar plot will be presented, with no patient marker or expected field visualized.

If no dedicated Liver images were received, a Liver Fat measurement cannot be calculated. This is indicated by a dash, “–”, instead of a value and a blank bar plot will be presented, with no patient marker or expected field visualized. A notification will be presented below the bar plot, to inform about this.

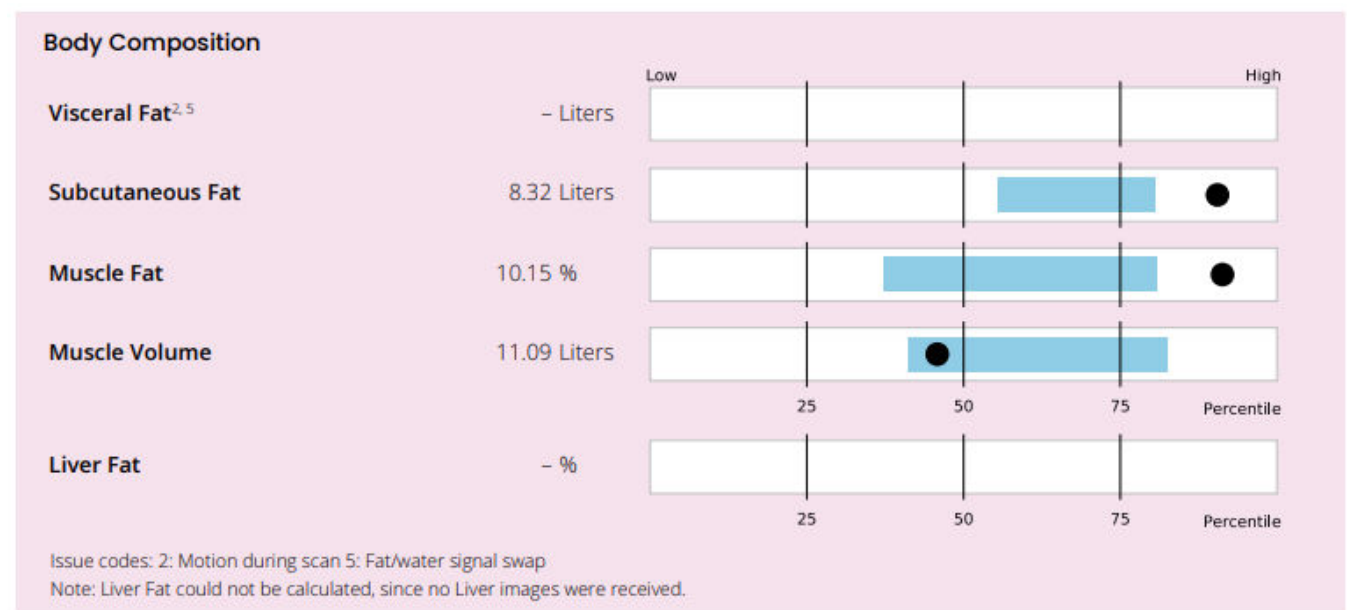

Example: Issues with the MRI scan resulting in that the Visceral Fat measurement could not be calculated within stated performance. A dash is output instead of a value and a blank bar plot is presented. The identified issues affecting the Visceral Fat measurement were Issue 2: “Motion during scan” and Issue 5: “Fat/water signal swap”. No Liver Fat value could be calculated, since no dedicated Liver images were received.

If there is an issue identified with the provided Patient Data, values will be presented, but a blank bar plot will be presented, with no patient marker or expected field visualized. A notification is presented at the bottom of the bar plot element, with a short description of the identified issue(s).

Single leg used in case of identified issue in one of the legs

Note: If there is an issue identified for one of the legs, only the leg without issues is used for muscle composition calculations in this element (Muscle Fat and Muscle Volume with corresponding bar plots). In such cases, a notification is presented, on which leg was used. This information can be of importance if comparing two BCP Scan reports from two different timepoints for the same patient. When this happens, it is also clear from the Detailed muscle composition section on page 2, that one of the legs could not be assessed.

3: Coronal Images

Representative coronal fat and water images of the patient, where the segmented volumes used to calculate the measurements are visualized with different colors. The color of each segmentation is explained in the image legend next to the images. This gives the reader an overview of the muscle and fat status within the patient's body.

In case there is an issue identified in the MRI data, resulting in that a measurement cannot be provided, no segmented volume is visualized for that region in the coronal images.

4: Detailed Muscle Composition

Measurements

The detailed muscle composition section presents the separate muscle composition values for the anterior and posterior thigh muscle groups as complementary information, allowing for assessment of differences in muscle composition between the legs.

Bar plots

Each muscle composition measurement is visualized in a bar plot to help put the patient's measurement in a relevant context. The patient's measurement (black dot) is compared to the distribution of measurements within a sex specific reference population (white bar). The 25th, 50th and 75th percentiles of this reference population are presented as solid lines. The distribution within the patient's virtual control group (blue bar) shows the expected range of the muscle measurement, given the provided patient's sex and body size.

Note: The patient marker being within the blue field, does not indicate if the patient is healthy or unhealthy.

Handling of identified input data issues

If issues in the MRI data are identified, the quality of the measurements cannot be guaranteed to be within the stated performance and the affected measurement(s) are therefore not reported. This is indicated by a dash, “–”, instead of a value and a blank bar plot will be presented, with no patient marker or expected field visualized.

If there is an issue identified with the provided Patient Data, values will be presented, but a blank bar plot will be presented, with no patient marker or expected field visualized. A notification is presented at the bottom of the bar plot element, with a short description of the identified issue.

5: Liver image

A representative slice of the liver is presented, with the ROIs placed in this slice visualized. The ROIs are a subset of the total number of ROIs used for calculation, which are evenly distributed within the liver. The image is either a Proton Density Fat Fraction (PDFF) image or a fat image, depending on which image was provided for Liver Fat calculations.

In case there is an issue identified in the MRI data of the liver, resulting in that a measurement cannot be provided, no ROIs are visualized in the Liver image.

Issue Categories Explained

Input data issues can occur either in the MRI data or in the Patient Data. The following sections explain more about the different issue categories. AMRA proposes remedial actions and how issues can be prevented going forward.

MRI Data Issues

Issue code	Short description given in report
1	Metal artifact
2	Motion during scan
3	Region partly outside field of view
4	Faulty alignment of adjacent slabs
5	Fat/water signal swap
6	Positive fat bias
10	Affected by strong negative fat signal
99	Other uncategorized issue

Table of issue categories used in AMRA® BCP Scan report to identify issues in the MRI data.

Issue 1: Metal artifact

The measurable region contains an imaging artifact specific to the presence of metal within the imaging volume, with an adverse effect on image quality. This can occur if the patient has a metal implant/prosthesis/device, metal in their clothing or jewelry/piercings have not been removed.

Remedial action: Rescan all sequences if the metal is removable. If the metal is an immovable implant, prosthesis, or device, no rescan of the patient shall be done.

To prevent recurrence: Ensure all patients are free from metallic objects, jewelry and piercings and that clothing is metal free, prior to MRI acquisition.

Issue 2: Motion during scan

The measurable region contains motion imaging artifacts, with an adverse effect on image quality. This can occur if any part of the patient's body moves during the scan.

Remedial action: Rescan all sequences.

To prevent recurrence: Ensure the patient remains as still as possible during the scan and repeat affected sequences at MRI acquisition, paying particular attention to the patient's compliance with breath-hold instructions.

Issue 3: Region partly outside field of view

The measurable region is wholly or partly outside of the imaging field of view. This can occur if the patient is not positioned correctly or has moved during or in-between sequences.

Remedial action: Rescan all sequences.

To prevent recurrence: Ensure the patient is positioned centered and straight on the scanner table. Ensure the arms and legs are not abducted from the body and air gaps between the limbs are minimized as far as site procedures allow. Take extra care to ensure the patient is not given any support underneath the legs. Prior to finalizing the scan, ensure the images contain all measurable anatomy. Repeat all sequences when improved patient positioning is deemed necessary.

Issue 4: Faulty alignment of adjacent slabs

The measurable region encompasses several incongruent or misaligned imaging slabs. This can occur when the MRI sequences are manually planned/angled, table positions altered, slice thickness/number altered, or the patient has changed position during or in-between sequences.

Remedial action: Rescan all sequences.

To prevent recurrence: Ensure table positions match those provided at protocol installation. Ensure the slabs are not manually planned or angled. Ensure the patient does not move or change position and complies with breath-hold instructions.

Issue 5: Fat/water signal swap

The measurable region contains an imaging artifact specific to a fat and water signal swap, with an adverse effect on image quality.

Remedial action: Rescan all sequences paying particular attention to MRI imaging artifacts at acquisition. If a fat/water swap is identified at acquisition, rescan any affected sequences.

To prevent recurrence: Ensure the patient is positioned centered and straight on the scanner table. Ensure the arms and legs are not abducted from the body and air gaps between the limbs are minimized as far as site procedures allow. Take extra care to ensure the patient is not given any supports underneath the legs and clothing is metal free.

Issue 6: Positive fat bias

The measurable region contains an area where the fat signal has a positive bias, which results in an erroneously elevated muscle fat infiltration measurement. This occurs mainly with Philips' scanners with software versions < 5.4 (not supported), but can, on rare occasions, happen with other scanners.

Remedial actions: If this issue occurs, please contact AMRA support for further guidance.

To prevent recurrence: If this issue occurs, please contact AMRA support for further guidance.

Issue 10: Affected by strong negative fat signal

The measurable region contains a strong negative fat signal close to, or within, the region of measurement, which results in erroneously lowered volume measurements. This issue can occur if there is iron present in the abdomen/intestines.

Remedial actions: None. The patient shall not be rescanned.

To prevent recurrence: None.

Issue 99: Other uncategorized issue

There is an issue with the MRI data that does not fit into any of the above categories. For more information on the issue that has occurred, please contact AMRA support.

Patient Data Issues

Issue code	Short description given in report
11	Missing patient data
12	Unreasonable height or weight

Table of issue categories used in AMRA® BCP Scan report to identify issues in the Patient Data.

Issue 11: Missing patient data

Required patient data height, weight, or sex, was not provided at upload to Ambra Health. The omitted patient data can be determined in the 'Patient Data' section of the report.

Remedial action: Add the missing patient data, either by re-uploading the images with corrected metadata (in case of upload is done via Ambra Gateway or Ambra Share Code) or add it manually to the examination in Ambra Webportal (in case of manual upload). Notify AMRA support that modification has been done, so that a re-analysis can be triggered and a new report generated. Always refer to the Patient ID when communicating with AMRA about a specific dataset.

Note that the patient shall not be rescanned.

To prevent recurrence: Ensure patient data is complete and accurate at upload. If any further guidance is needed, please contact AMRA support.

Issue 12: Unreasonable height or weight

BMI calculated from the input height and weight value is outside the interval of 10-100 kg/m². This can occur if incorrect values are input at upload to Ambra Health or the values are not represented in conventional SI units.

Remedial action: Check the height and weight values presented in the 'Patient Data' section of the report and update the numbers to the correct values, either by re-uploading the examination with corrected metadata (in case of upload via Ambra Gateway or Ambra Share Code) or modify it manually for the examination in Ambra Webportal (in case of manual upload). Notify AMRA support that patient data has been modified, so that a re-analysis can be triggered and a new report generated. Always refer to the Patient ID when communicating with AMRA about a specific dataset.

Note that the patient shall not be rescanned.

To prevent recurrence: Ensure patient height and weight are correct at upload. If any further guidance is needed, please contact AMRA support.

Machine-readable Format

There is an option to get the information from the BCP Scan report delivered on a machine-readable format (JSON), in addition to the PDF report. If this is of interest, contact AMRA support at support@amramedical.com for more information.

Note: The content of the machine-readable file shall always be used in conjunction with the PDF report delivered at the same time.

Reference Population Characteristics

	Total	Females	Males
N	30176 (100.0%)	15631 (51.8%)	14545 (48.2%)
Age (years)	64.7 (7.5)	64.1 (7.3)	65.4 (7.6)
Race [White] (No.)	29136 (96.6%)	15099 (96.6%)	14037 (96.5%)
Race [Black] (No.)	229 (0.8%)	130 (0.8%)	99 (0.7%)
Race [Asian] (No.)	354 (1.2%)	134 (0.9%)	220 (1.5%)
Race [Chinese] (No.)	95 (0.3%)	60 (0.4%)	35 (0.2%)
Race [Mixed] (No.)	139 (0.5%)	90 (0.6%)	49 (0.3%)
Race [Other] (No.)	154 (0.5%)	86 (0.6%)	68 (0.5%)
Weight (kg)	76.0 (15.2)	68.9 (13.1)	83.6 (13.4)
Height (cm)	169.5 (9.2)	163.0 (6.2)	176.4 (6.6)
Body mass index (kg/m ²)	26.4 (4.4)	25.9 (4.7)	26.8 (3.9)
Waist circumference (cm)	88.7 (12.8)	83.1 (12.0)	94.6 (10.9)
Visceral Fat (L)	3.8 (2.3)	2.7 (1.5)	4.9 (2.4)
Subcutaneous Fat (L)	6.9 (3.2)	7.9 (3.4)	5.9 (2.5)
Liver Fat (%)	4.3 (4.0)	3.9 (3.8)	4.8 (4.1)
Muscle Volume (L)	10.2 (2.5)	8.2 (1.2)	12.3 (1.8)
Muscle Volume Index (SD)	0.0 (1.0)	0.0 (1.0)	0.0 (1.0)
Muscle Fat (%)	8.3 (2.0)	9.0 (1.9)	7.6 (1.9)
Muscle Fat Index (pp)	0.3 (1.9)	0.3 (1.9)	0.3 (1.9)
Left Anterior Thigh Muscle Volume (L)	1.7 (0.5)	1.3 (0.2)	2.1 (0.4)
Right Anterior Thigh Muscle Volume (L)	1.7 (0.5)	1.3 (0.2)	2.1 (0.4)
Left Posterior Thigh Muscle Volume (L)	3.4 (0.8)	2.7 (0.4)	4.0 (0.6)
Right Posterior Thigh Muscle Volume (L)	3.4 (0.8)	2.8 (0.4)	4.1 (0.6)
Left Anterior Thigh Muscle Fat (%)	8.4 (2.1)	9.1 (2.0)	7.6 (1.9)
Right Anterior Thigh Muscle Fat (%)	8.3 (2.1)	9.0 (2.0)	7.6 (2.0)
Left Posterior Thigh Muscle Fat (%)	12.2 (2.5)	12.9 (2.4)	11.4 (2.4)
Right Posterior Thigh Muscle Fat (%)	11.9 (2.5)	12.6 (2.4)	11.2 (2.4)
Metabolic disease free (No.)	7278 (24.1%)	3774 (24.1%)	3504 (24.1%)
Non-alcoholic fatty liver disease (No.)	3860 (12.8%)	1814 (11.6%)	2046 (14.1%)
Diabetes, type 2 (No.)	1557 (5.2%)	510 (3.3%)	1047 (7.2%)
Cardiovascular disease (No.)	2004 (6.6%)	535 (3.4%)	1469 (10.1%)
Coronary heart disease (No.)	1586 (5.3%)	402 (2.6%)	1184 (8.1%)
Cancer (No.)	3177 (10.5%)	1747 (11.2%)	1430 (9.8%)

Reference population characteristics. Values are mean (standard deviations).

Performance Specification

Measurement	Accuracy	Precision	Reproducibility
Liver Fat	±2.0 pp	1.0 pp	2.0 pp
Visceral Fat	Volume and muscle fat measurements are to be compared to the provided reference intervals	0.10 L	0.15 L
Subcutaneous Fat		0.20 L	0.25 L
Muscle Volume		0.15 L	0.20 L
Left/Right Anterior/Posterior Thigh Muscle Volumes		0.05 L	0.10 L
Thigh Muscle Fat		0.5 pp	1.0 pp
Left/Right Anterior/Posterior Thigh Muscle Fat		0.5 pp	1.0 pp

L – Liter, pp – percentage point, SD – Standard Deviation.

Performance is derived from in-vivo experiments and represents limits of performance - measured performance is normally within the limits. Liver Fat represents AMRA's fat-referenced Liver Fat method. Accuracy was assessed by comparison with established reference methods, precision using a test-retest design, and reproducibility by scanning the same subjects on multiple different MRI systems. Accuracy is reported as outer limits of the limits of agreement, while precision and reproducibility are reported as upper limits of the within-subject standard deviation.

Appendix A: Input of Patient Height on GE or Philips MRI Consoles

When registering the patient for the AMRA[®] BCP Scan Protocol, please insert the patient's height into the following fields on the MRI console:

GE: Additional Patient History (0010,21B0)

Philips: Study Comments (0032,4000)

Input the height in either meters or inches:

Meters: Type "HEIGHT *number* METERS", for example "HEIGHT 1.84 METERS"

Inches: Type "HEIGHT *number* INCHES", for example "HEIGHT 72.4 INCHES"

To convert feet into inches, multiply height in feet with 12.

For support, contact support@amramedical.com